



[Go to Product page](#)

Datasheet for ABIN1979526

## MBP/MBL ELISA Kit

### 1 Image

#### Overview

Quantity:	96 tests
Target:	MBP/MBL
Reactivity:	Human
Method Type:	Sandwich ELISA
Detection Range:	0.03-25 ng/mL
Minimum Detection Limit:	0.03 ng/mL
Application:	ELISA

#### Product Details

Purpose:	Human MBL ELISA Kit for cell culture supernatants, plasma, and serum samples.
Sample Type:	Plasma, Cell Culture Supernatant, Serum
Analytical Method:	Quantitative
Detection Method:	Colorimetric
Specificity:	This ELISA antibody pair detects human MBL. Other species not determined yet.
Characteristics:	<ul style="list-style-type: none"><li>• Strip plates and additional reagents allow for use in multiple experiments</li><li>• Quantitative protein detection</li><li>• Establishes normal range</li><li>• The best products for confirmation of antibody array data</li></ul>
Components:	<ul style="list-style-type: none"><li>• Pre-Coated 96-well Strip Microplate</li><li>• Wash Buffer</li><li>• Stop Solution</li></ul>

## Product Details

---

- Assay Diluent(s)
- Lyophilized Standard
- Biotinylated Detection Antibody
- Streptavidin-Conjugated HRP
- TMB One-Step Substrate

---

### Material not included:

- Distilled or deionized water
- Precision pipettes to deliver 2 µL to 1 µL volumes
- Adjustable 1-25 µL pipettes for reagent preparation
- 100 µL and 1 liter graduated cylinders
- Tubes to prepare standard and sample dilutions
- Absorbent paper
- Microplate reader capable of measuring absorbance at 450nm
- Log-log graph paper or computer and software for ELISA data analysis

## Target Details

---

Target: MBP/MBL

Alternative Name: MBL ([MBP/MBL Products](#))

Gene ID: 4153

UniProt: [P11226](#)

## Application Details

---

Application Notes: Recommended Dilution for serum and plasma samples 800 fold

Sample Volume: 100 µL

Plate: Pre-coated

Protocol:

1. Prepare all reagents, samples and standards as instructed in the manual.
2. Add 100 µL of standard or sample to each well.
3. Incubate 2.5 h at RT or O/N at 4 °C.
4. Add 100 µL of prepared biotin antibody to each well.
5. Incubate 1 h at RT.
6. Add 100 µL of prepared Streptavidin solution to each well.
7. Incubate 45 min at RT.
8. Add 100 µL of TMB One-Step Substrate Reagent to each well.
9. Incubate 30 min at RT.
10. Add 50 µL of Stop Solution to each well.
11. Read at 450 nm immediately.

---

## Application Details

---

**Reagent Preparation:**

1. Bring all reagents and samples to room temperature (18 - 25 °C) before use.
2. Sample dilution: If your samples need to be diluted, Assay Diluent A (Item D) should be used for dilution of serum/plasma samples. 1x Assay Diluent B (Item E) should be used for dilution of culture supernatants and urine. Suggested dilution for normal serum/plasma: 800 fold\*. The Human MBL ELISA Kit Protocol 3 \* Please note that levels of the target protein may vary between different specimens. Optimal dilution factors for each sample must be determined by the investigator.
3. Assay Diluent B should be diluted 5-fold with deionized or distilled water before use.
4. Preparation of standard: Briefly spin the vial of Item C and then add 800 µL Assay Diluent A (for serum/plasma samples) or 1x Assay Diluent B (for cell culture supernates/urine) into Item C vial to prepare a 25 ng/ml standard. Dissolve the powder thoroughly by a gentle mix. Pipette 400 µL Assay Diluent A or 1x Assay Diluent B into each tube. Use the 25 ng/ml standard solution to produce a dilution series (shown below). Mix each tube thoroughly before the next transfer. Assay Diluent A or 1x Assay Diluent B serves as the zero standard (0 ng/ml).

200 µL Standard, Item C + 800 µL	200µml	200 µL	200 µL	200 µL	200 µL	25	8.333	2.778	0.926	0.309	0.103	0.034	0 ng/ml	ng/ml	ng/ml	ng/ml	ng/ml	ng/ml	ng/ml	ng/ml
----------------------------------	--------	--------	--------	--------	--------	----	-------	-------	-------	-------	-------	-------	---------	-------	-------	-------	-------	-------	-------	-------
5. If the Wash Concentrate (20x) (Item B) contains visible crystals, warm to room temperature and mix gently until dissolved. Dilute 20 mL of Wash Buffer Concentrate into deionized or distilled water to yield 400 mL of 1x Wash Buffer.
6. Briefly spin the Detection Antibody vial (Item F) before use. Add 100 µL of 1x Assay Diluent B into the vial to prepare a detection antibody concentrate. Pipette up and down to mix gently (the concentrate can be stored at 4 °C for 5 days). The detection antibody concentrate should be The Human MBL ELISA Kit Protocol 4 diluted 80-fold with 1x Assay Diluent B and used in step 4 of Part VI Assay Procedure.
7. Briefly spin the HRP-Streptavidin concentrate vial (Item G) and pipette up and down to mix gently before use. HRP-Streptavidin concentrate should be diluted 800-fold with 1x Assay Diluent B. For example: Briefly spin the vial (Item G) and pipette up and down to mix gently . Add 15 µL of HRP-Streptavidin concentrate into a tube with 12 mL 1x Assay Diluent B to prepare a 800-fold diluted HRP- Streptavidin solution (don't store the diluted solution for next day use). Mix well.

**Assay Procedure:**

1. Bring all reagents and samples to room temperature (18 - 25 °C) before use. It is recommended that all standards and samples be run at least in duplicate.
2. Add 100 µL of each standard (see Reagent Preparation step 2) and sample into appropriate wells. Cover well and incubate for 2.5 hours at room temperature or over night at 4 °C with gentle shaking.
3. Discard 5. Discard the solution. Repeat the wash as in step 3.
6. Add 100 µL of prepared Streptavidin solution (see Reagent Preparation step 7) to each well. Incubate for 45 minutes at room temperature with gentle shaking.
7. Discard the solution. Repeat the wash as in step 3.
8. Add 100 µL of TMB One-Step Substrate Reagent (Item H) to each well. Incubate for 30 minutes

## Application Details

at room temperature in the dark with gentle shaking. 9. Add 50  $\mu$ L of Stop Solution (Item I) to each well. Read at 450 nm immediately.

**Calculation of Results:** Calculate the mean absorbance for each set of duplicate standards, controls and samples, and subtract the average zero standard optical density. Plot the standard curve on log-log graph paper or using Sigma plot software, with standard concentration on the x-axis and absorbance on the y-axis. Draw the best-fit straight line through the standard points.

**Assay Precision:** Intra-Assay: CV<10%  
Inter-Assay: CV<12%

**Restrictions:** For Research Use only

## Handling


**Handling Advice:** Avoid repeated freeze-thaw cycles.

**Storage:** -20 °C

**Storage Comment:** The entire kit may be stored at -20°C for up to 1 year from the date of shipment. Avoid repeated freeze-thaw cycles. The kit may be stored at 4°C for up to 6 months. For extended storage, it is recommended to store at -80°C.

**Expiry Date:** 6 months

## Images

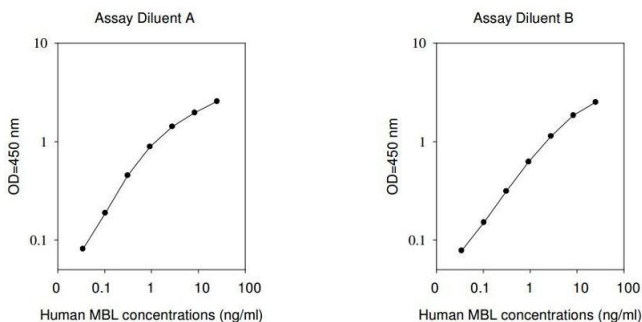

### ELISA

#### Image 1.