



[Go to Product page](#)

Datasheet for ABIN4886397

Trastuzumab ELISA Kit

1 Image

Overview

Quantity:	96 tests
Target:	Trastuzumab
Reactivity:	Human, Mouse, Rat
Method Type:	Sandwich ELISA
Detection Range:	1.25-40 ng/mL
Minimum Detection Limit:	1.25 ng/mL
Application:	ELISA

Product Details

Purpose:	Quantification of Trastuzumab in biological matrices
Sample Type:	Plasma, Serum
Analytical Method:	Quantitative
Detection Method:	Colorimetric
Specificity:	Trastuzumab (Herceptin)
Cross-Reactivity (Details):	hIgG1, Rituximab, and Infliximab prepared at 250 ng/mL were assayed and exhibited no cross-reactivity or interference.
Components:	Coated microtiter plate, 96 wells Calibrator diluent. - 1.8ml Calibrator 12ul 10X wash buffer - 25ml Assay buffer - 50ml

Product Details

1000X detection reagent - 17ul

TMB - 12ml

TMB stop solution - 12ml

Plate sealers - 3

Material not included:

- Precision pipettes calibrated to deliver 5-1000µL
- Multi-channel pipette calibrated to deliver 50-200µL
- Plate shaker
- Disposable tips
- Vortex-Mixer
- Distilled or de-ionized water
- Microplate reader capable of reading 450nm with background subtrac

Target Details

Target: Trastuzumab

Abstract: [Trastuzumab Products](#)

Background: Trastuzumab (Herceptin®) is indicated for the treatment of HER2-positive breast cancer, and adjuvant therapies for metastatic gastric cancer and gastroesophageal cancer. Serum concentration of Trastuzumab may predict some clinical outcome during therapy. It is also possible that the surveillance of circulating Trastuzumab concentration during therapy represents a direct factor for immunogenicity and some other side effects. Identification of biomarkers and risk factors for adverse drug reactions that might be related to serum concentrations, and maintaining the effective minimum concentration of Trastuzumab in order to potentially avoid some side effects, might be beneficial using a reliable method

Gene ID: 2064

Application Details

Application Notes: Optimal working dilution should be determined by the investigator.

Sample Volume: 15 µL

Assay Time: 2.5 h

Plate: Pre-coated

Protocol: The Trastuzumab ELISA kit is designed to measure free Trastuzumab with high specificity and sensitivity . This assay employs the sandwich enzyme immunoassay technique. A precoated

Application Details

anti-Trastuzumab 96 well plate is provided. Calibrator, quality control samples and test samples are pipetted into the appropriate wells. Trastuzumab present in biological matrices is bound by the immobilized capture antibody. After washing away any unbound substances, enzyme linked detection antibody is added to the wells. The plate is washed to remove any unbound antibody-enzyme reagent and a substrate solution is added to the wells for color development. The color development is proportional to the amount of Trastuzumab present in test samples and the concentration is calculated from the standard series.

Reagent Preparation: Prepare only the appropriate amount of required reagent on the day of use. Store all reagents as per instructions stated on the label. 1. Wash Buffer (1X) Preparation: Dilute wash buffer concentrate with ultra-pure water 1/10 before use (for example add 10 mL concentrate to 90 mL ultra-pure water). Mix well. 2. Detection Reagent (1X) Preparation: Dilute detection reagent with assay buffer 1/1000 before use (for example add 10 μ L concentrate to 10 mL of assay buffer). Mix well. 3. Preparation of Calibrators: Prepare calibrators with concentrations ranging from 1000 ng/mL to 62.5 ng/mL. The following is an example calibrator curve.

Sample Collection: This kit is compatible with EDTA-plasma, heparinplasma and serum samples. Samples can be stored at or below -20 °C for up to 1 year.

Sample Preparation: Dilute calibrators and test samples 1/50 with assay buffer (for example add 5 μ L of prepared calibrator or sample to 245 μ L of assay buffer). Mix well. Do not store diluted samples.

Assay Procedure: This assay employs the sandwich enzyme immunoassay technique. Anti- Trastuzumab is coated onto a 96 well microplate. Calibrator, quality control samples (if desired) and test samples are pipetted into the appropriate wells. Trastuzumab present in biological matrices is bound by the immobilized anti- Trastuzumab antibody. After washing away any unbound substances, enzyme linked antiTrastuzumab antibody is added to the wells. The plate is washed to remove any unbound antibody-enzyme reagent and a substrate solution is added to the wells for color development. The color development is proportional to the amount of Trastuzumab present in test samples. The color development is stopped and the intensity of the color is measured.

Calculation of Results: 1. Construct a standard curve by plotting the absorbance obtained from each standard against concentration. Use a 4 or 5 parameter curve fit. Alternatively a log-log curve fit may be used. 2. The concentration of the unknowns can be read directly from this standard curve using the absorbance value for each sample. 3. Any sample undiluted or diluted still reading greater than the highest standard should be diluted appropriately with calibrator diluent and retested. If the samples have been diluted, the concentration determined from the standard curve must be multiplied by the dilution factor.


Application Details

Assay Precision:	Precision: The precision was determined by analyzing samples prepared at 1000 ng/mL in 6 replicates on 6 different occasions. Intra-assay coefficient of variation (CV) < 10%. Inter-assay CV < 10%.
	Recovery: 1000ng/mL of Trastuzumab was spiked in 10 lots of human serum. Recovery ranges are from 91-117% with an average recovery of 106%.
Restrictions:	For Research Use only

Handling

Preservative:	Without preservative
Precaution of Use:	Read manual completely before beginning
Storage:	-20 °C
Storage Comment:	Store kit components at -20°C unless specified otherwise. DO NOT USE past kit expiration date. Some vials contain a small amount of reagents. Spin tubes on pulse setting prior to opening.
Expiry Date:	12 months

Images

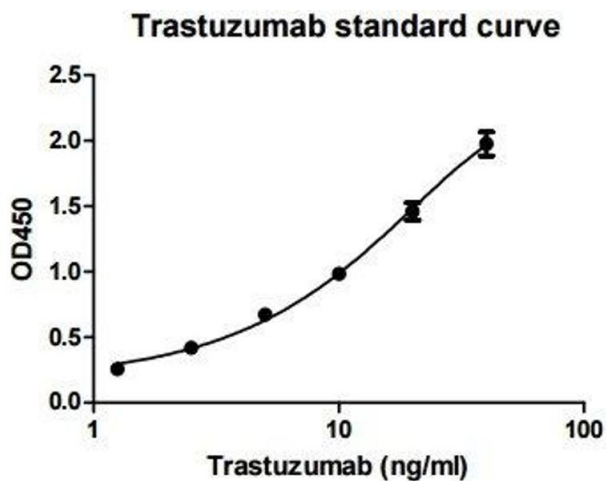

ELISA

Image 1.