

Datasheet for ABIN625002

IGFBP6 ELISA Kit[Go to Product page](#)**1** Image**2** Publications

Overview

| | |
|--------------------------|-----------------|
| Quantity: | 96 tests |
| Target: | IGFBP6 |
| Reactivity: | Human |
| Method Type: | Sandwich ELISA |
| Detection Range: | 150-60000 pg/mL |
| Minimum Detection Limit: | 150 pg/mL |
| Application: | ELISA |

Product Details

| | |
|--------------------|--|
| Purpose: | Human IGFBP-6 ELISA Kit for cell culture supernatants, plasma, and serum samples. |
| Sample Type: | Plasma, Cell Culture Supernatant, Serum |
| Analytical Method: | Quantitative |
| Detection Method: | Colorimetric |
| Specificity: | This ELISA kit shows no cross-reactivity with any of the cytokines tested: Human Angiogenin, BDNF, BLC, ENA-78, FGF-4, IL-1 alpha, IL-1 beta, IL-2, IL-3, IL-4, IL-5, IL-7, IL-8, IL-9, IL-10, IL-11, IL-12 p70, IL-12 p40, IL-13, IL-15, I-309, IP-10, G-CSF, GM-CSF, IFN-gamma, IGFBP-1, IGFBP-2, IGFBP-3, IGFBP-4, Leptin, MCP-1, MCP-2, MCP-3, MDC, MIP-1 alpha, MIP-1 beta, MIP-1 delta, PARC, PDGF, RANTES, SCF, TARC, TGF-beta, TIMP-1, TIMP-2, TNF-alpha, TNF-beta, TPO, VEGF. |
| Sensitivity: | 150 pg/mL |
| Characteristics: | <ul style="list-style-type: none">• Strip plates and additional reagents allow for use in multiple experiments |

Product Details

- Quantitative protein detection
- Establishes normal range
- The best products for confirmation of antibody array data

- Components:
- Pre-Coated 96-well Strip Microplate
 - Wash Buffer
 - Stop Solution
 - Assay Diluent(s)
 - Lyophilized Standard
 - Biotinylated Detection Antibody
 - Streptavidin-Conjugated HRP
 - TMB One-Step Substrate

- Material not included:
- Distilled or deionized water
 - Precision pipettes to deliver 2 μ L to 1 μ L volumes
 - Adjustable 1-25 μ L pipettes for reagent preparation
 - 100 μ L and 1 liter graduated cylinders
 - Tubes to prepare standard and sample dilutions
 - Absorbent paper
 - Microplate reader capable of measuring absorbance at 450nm
 - Log-log graph paper or computer and software for ELISA data analysis

Target Details

Target: IGFBP6

Alternative Name: IGFBP-6 ([IGFBP6 Products](#))

Background: IGF-BPs (Insulin-like growth factor binding proteins) are found in various body fluids such as blood serum, amniotic fluid, and liquor. They are synthesized in the liver and are produced also by various tumor cell lines and cell types. Human IGFBP6 is an O-glycosylated protein. It is abundant in cerebrospinal fluid and has a marked preferential binding affinity for IGF-2 over IGF-1. Levels of IGFBP6 have been found to be increased in human breast cancer cells treated with estradiol and IGF-1 and may thus contribute to mitogenesis. The Human IGF-BP-6 ELISA (Enzyme-Linked Immunosorbent Assay) kit is an in vitro enzyme-linked immunosorbent assay for the quantitative measurement of human IGF-BP-6 in serum, plasma, cell culture supernatants and urine. This assay employs an antibody specific for human IGF-BP-6 coated on a 96-well plate. Standards and samples are pipetted into the wells and IGF-BP-6 present in a sample is bound to the wells by the immobilized antibody. The wells are washed and biotinylated anti-human IGF-BP-6 antibody is added. After washing away unbound biotinylated antibody, HRP-conjugated streptavidin is pipetted to the wells. The wells are again washed, a

Target Details

TMB substrate solution is added to the wells and color develops in proportion to the amount of IGF-BP-6 bound. The Stop Solution changes the color from blue to yellow, and the intensity of the color is measured at 450 nm. Reproducibility: Intra-Assay: CV<10% Inter-Assay: CV<12%.

Gene ID: 3489

UniProt: [P24592](#)

Pathways: [WNT Signaling, Myometrial Relaxation and Contraction](#)

Application Details

Application Notes: Recommended Dilution for serum and plasma samples 20 - 500 fold

Sample Volume: 100 µL

Plate: Pre-coated

Protocol:

1. Prepare all reagents, samples and standards as instructed in the manual.
2. Add 100 µL of standard or sample to each well.
3. Incubate 2.5 h at RT or O/N at 4 °C.
4. Add 100 µL of prepared biotin antibody to each well.
5. Incubate 1 h at RT.
6. Add 100 µL of prepared Streptavidin solution to each well.
7. Incubate 45 min at RT.
8. Add 100 µL of TMB One-Step Substrate Reagent to each well.
9. Incubate 30 min at RT.
10. Add 50 µL of Stop Solution to each well.
11. Read at 450 nm immediately.

Reagent Preparation:

1. Bring all reagents and samples to room temperature (18 - 25°C) before use.
2. Sample dilution: If your samples need to be diluted, Assay Diluent A (Item D) is used for dilution of serum/plasma samples, and Assay Diluent B (Item E) is used for dilution of culture supernatants and urine.
3. Assay Diluent B should be diluted 5-fold with deionized or distilled water.
4. Preparation of standard: Briefly spin the vial of Item C and then add 400 µl Assay Diluent A (for serum/plasma samples) or 1x Assay Diluent B (for cell culture medium and urine, Assay Diluent B should be diluted 5-fold with deionized or distilled water before use) into Item C vial to prepare a 200 ng/ml standard. Dissolve the powder thoroughly by a gentle mix. Add 180 µl IGF-BP-6 standard from the vial of Item C, into a tube with 420 µl Assay Diluent A or 1x Assay Diluent B to prepare a 60,000 pg/ml stock standard solution. Pipette 400 µl Assay Diluent A or 1x Assay Diluent B into each tube. Use the stock standard solution to produce a dilution series (shown below). Mix each tube thoroughly before the next transfer. Assay Diluent A or 1x Assay

Diluent B serves as the zero standard (0 pg/ml). 5. If the Wash Concentrate (20x) (Item B) contains visible crystals, warm to room temperature and mix gently until dissolved. Dilute 20 ml of Wash Buffer Concentrate into deionized or distilled water to yield 400 ml of 1x Wash Buffer. 6. Briefly spin the Detection Antibody vial (Item F) before use. Add 100 µl of 1x Assay Diluent B into the vial to prepare a detection antibody concentrate. Pipette up and down to mix gently (the concentrate can be stored at 4°C for 5 days). The detection antibody concentrate should be diluted 80-fold with 1x Assay Diluent B and used in step 4 of Part VI Assay Procedure. 7. Briefly spin the HRP-Streptavidin concentrate vial (Item G) and pipette up and down to mix gently before use. HRP- Streptavidin concentrate should be diluted 25,000-fold with 1x Assay Diluent B. For example: Briefly spin the vial (Item G) and pipette up and down to mix gently . Add 2 µl of HRP-Streptavidin concentrate into a tube with 198.0 µl 1x Assay Diluent B to prepare a 100-fold diluted HRP- Streptavidin solution (do not store the diluted solution for next day use). Mix through and then pipette 40 µl of prepared 100-fold diluted solution into a tube with 10 ml 1x Assay Diluent B to prepare a final 25,000 fold diluted HRP-Streptavidin solution.

Assay Procedure:

1. Bring all reagents and samples to room temperature (18 - 25°C) before use. It is recommended that all standards and samples be run at least in duplicate. 2. Add 100 µl of each standard (see Reagent Preparation step 2) and sample into appropriate wells. Cover well and incubate for 2.5 hours at room temperature or over night at 4°C with gentle shaking. 3. Discard the solution and wash 4 times with 1x Wash Solution. Wash by filling each well with Wash Buffer (300 µl) using a multi-channel Pipette or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels. 4. Add 100 µl of 1x prepared biotinylated antibody (Reagent Preparation step 6) to each well. Incubate for 1 hour at room temperature with gentle shaking. 5. Discard the solution. Repeat the wash as in step 3. 6. Add 100 µl of prepared Streptavidin solution (see Reagent Preparation step 7) to each well. Incubate for 45 minutes at room temperature with gentle shaking. 7. Discard the solution. Repeat the wash as in step 3. 8. Add 100 µl of TMB One-Step Substrate Reagent (Item H) to each well. Incubate for 30 minutes at room temperature in the dark with gentle shaking. 9. Add 50 µl of Stop Solution (Item I) to each well. Read at 450 nm immediately.

Calculation of Results:

Calculate the mean absorbance for each set of duplicate standards, controls and samples, and subtract the average zero standard optical density. Plot the standard curve on log-log graph paper or using Sigma plot software, with standard concentration on the x-axis and absorbance on the y-axis. Draw the best-fit straight line through the standard points.

Restrictions:

For Research Use only

Handling

Storage: -20 °C

Storage Comment: The entire kit may be stored at -20°C for up to 1 year from the date of shipment. Avoid repeated freeze-thaw cycles. The kit may be stored at 4°C for up to 6 months. For extended storage, it is recommended to store at -80°C.


Expiry Date: 6 months

Publications

Product cited in: Sawada, Takedachi, Yamamoto, Morimoto, Ozasa, Iwayama, Lee, Okura, Matsuyama, Kitamura, Murakami: "Trophic factors from adipose tissue-derived multi-lineage progenitor cells promote cytodifferentiation of periodontal ligament cells." in: **Biochemical and biophysical research communications**, Vol. 464, Issue 1, pp. 299-305, (2015) ([PubMed](#)).

Liu, Liu, Zhou, Xiao, Cao: "Conditioned medium from chondrocyte/scaffold constructs induced chondrogenic differentiation of bone marrow stromal cells." in: **Anatomical record (Hoboken, N.J. : 2007)**, Vol. 295, Issue 7, pp. 1109-16, (2012) ([PubMed](#)).

Images

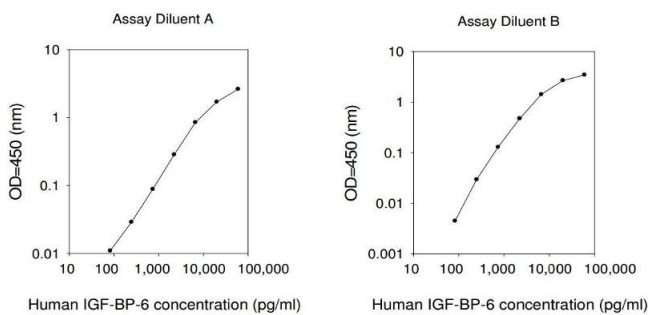

ELISA

Image 1.