.-online.com antibodies

Datasheet for ABIN6953933 ARNT ELISA Kit

Image



Overview

Quantity:	96 tests
Target:	ARNT
Reactivity:	Human
Method Type:	Sandwich ELISA
Detection Range:	0.15 ng/mL - 10 ng/mL
Minimum Detection Limit:	0.15 ng/mL
Application:	ELISA

Product Details

human serum, plasma, tissue homogenates, cell lysates, cell culture supernates.Sample Type:Cell Culture Supernatant, Cell Lysate, Plasma, Serum, Tissue HomogenateAnalytical Method:QuantitativeDetection Method:ColorimetricSpecificity:This assay has high sensitivity and excellent specificity for detection of Aryl Hydrocarbon Receptor Nuclear Translocator (ARNT)Sensitivity:0.054 ng/mLComponents:• Pre-coated, ready to use 96-well strip plate, flat buttom • Plate sealer for 96 wells		
Analytical Method: Quantitative Detection Method: Colorimetric Specificity: This assay has high sensitivity and excellent specificity for detection of Aryl Hydrocarbon Receptor Nuclear Translocator (ARNT) Sensitivity: 0.054 ng/mL Components: • Pre-coated, ready to use 96-well strip plate, flat buttom • Plate sealer for 96 wells	Purpose:	The kit is a sandwich enzyme immunoassay for in vitro quantitative measurement of ARNT in human serum, plasma, tissue homogenates, cell lysates, cell culture supernates.
Detection Method:ColorimetricSpecificity:This assay has high sensitivity and excellent specificity for detection of Aryl Hydrocarbon Receptor Nuclear Translocator (ARNT)Sensitivity:0.054 ng/mLComponents:• Pre-coated, ready to use 96-well strip plate, flat buttom • Plate sealer for 96 wells	Sample Type:	Cell Culture Supernatant, Cell Lysate, Plasma, Serum, Tissue Homogenate
Specificity: This assay has high sensitivity and excellent specificity for detection of Aryl Hydrocarbon Receptor Nuclear Translocator (ARNT) Sensitivity: 0.054 ng/mL Components: • Pre-coated, ready to use 96-well strip plate, flat buttom • Plate sealer for 96 wells	Analytical Method:	Quantitative
Receptor Nuclear Translocator (ARNT) Sensitivity: 0.054 ng/mL Components: • Pre-coated, ready to use 96-well strip plate, flat buttom • Plate sealer for 96 wells	Detection Method:	Colorimetric
Components: • Pre-coated, ready to use 96-well strip plate, flat buttom • Plate sealer for 96 wells	Specificity:	This assay has high sensitivity and excellent specificity for detection of Aryl Hydrocarbon Receptor Nuclear Translocator (ARNT)
Plate sealer for 96 wells	Sensitivity:	0.054 ng/mL
Reference Standard	Components:	Plate sealer for 96 wellsReference Standard

• Standard Diluent

Order at www.antibodies-online.com | www.antikoerper-online.de | www.anticorps-enligne.fr | www.antibodies-online.cn International: +49 (0)241 95 163 153 | USA & Canada: +1 877 302 8632 | support@antibodies-online.com Page 1/5 | Product datasheet for ABIN6953933 | 09/10/2023 | Copyright antibodies-online. All rights reserved.

- Detection Reagent A
- Detection Reagent B
- Assay Diluent A
- Assay Diluent B
- Reagent Diluent (if Detection Reagent is lyophilized)
- TMB Substrate
- Stop Solution
- Wash Buffer (30 x concentrate)
- Instruction manual

Target Details

Target:	ARNT
Abstract:	ARNT Products
Pathways:	Regulation of Hormone Metabolic Process, Regulation of Hormone Biosynthetic Process, Regulation of Carbohydrate Metabolic Process, Signaling Events mediated by VEGFR1 and
	VEGFR2, Warburg Effect

Application Details

Comment:	Information on standard material:
	The standard might be recombinant protein or natural protein, that will depend on the specific
	kit. Moreover, the expression system is E.coli or yeast or mammal cell. There is 0.05% proclin
	300 in the standard as preservative.
	Information on reagents:
	The stop solution used in the kit is sulfuric acid with concentration of 1 mol/L. And the wash
	solution is TBS. The standard diluent contains 0.02 % sodium azide, assay diluent A and assay
	diluent B contain 0.01% sodium azide. Some kits can contain is BSA in them.
	Information on antibodies:
	The provided antibodies and their host vary in different kits.
Sample Volume:	100 μL
Assay Time:	3 h
Plate:	Pre-coated

Order at www.antibodies-online.com | www.antikoerper-online.de | www.anticorps-enligne.fr | www.antibodies-online.cn International: +49 (0)241 95 163 153 | USA & Canada: +1 877 302 8632 | support@antibodies-online.com Page 2/5 | Product datasheet for ABIN6953933 | 09/10/2023 | Copyright antibodies-online. All rights reserved.

Application Details


Protocol:	1. Prepare all reagents, samples and standards, 2. Add 100µL standard or sample to each well. Incubate 1 hours at 37 °C,
	3. Aspirate and add 100 μ L prepared Detection Reagent A. Incubate 1 hour at 37 °C,
	4. Aspirate and wash 3 times,
	5. Add 100µL prepared Detection Reagent B. Incubate 30 minutes at 37 °C,
	6. Aspirate and wash 5 times,
	7. Add 90µL Substrate Solution. Incubate 10-20 minutes at 37 °C,
	8. Add 50µL Stop Solution. Read at 450nm immediately.
Reagent Preparation:	1. Bring all kit components and samples to room temperature (18-25 °C) before use. If the kit
	will not be used up in one time, please only take out strips and reagents for present experiment, and leave the remaining strips and reagents in required condition.
	2. Standard - Reconstitute the Standard with 1.0 mL of Standard Diluent, keep for 10 minutes at
	room temperature, shake gently (not to foam). The concentration of the standard in the stock solution is 20 ng/mL. Firstly dilute the stock solution to 10 ng/mL and the diluted standard
	serves as the highest standard (10 ng/mL). Then prepare 7 tubes containing 0.5 mL
	Standard Diluent and use the diluted standard to produce a double dilution series. Mix each
	tube thoroughly before the next transfer. Set up 7 points of diluted standard such as
	10 ng/mL, 5 ng/mL, 2.5 ng/mL, 1.25 ng/mL, 0.625 ng/mL, 0.312 ng/mL, 0.156 ng/mL, and
	the last microcentrifuge tube with Standard Diluent is the blank as 0 ng/mL.
	3. Detection Reagent A and Detection Reagent B - If lyophilized reconstitute the Detection
	Reagent A with 150 μ L of Reagent Diluent, keep for 10 minutes at room temperature, shake
	gently (not to foam). Briefly spin or centrifuge the stock Detection A and Detection B before
	use. Dilute them to the working concentration 100-fold with Assay Diluent A and B,
	respectively.
	4. Wash Solution - Dilute 20 mL of Wash Solution concentrate (30x) with 580 mL of deionized
	or distilled water to prepare 600 mL of Wash Solution (1x).
	5. TMB substrate - Aspirate the needed dosage of the solution with sterilized tips and do not
	dump the residual solution into the vial again.
	Note:
	1. Making serial dilution in the wells directly is not permitted.
	2. Prepare standards within 15 minutes before assay. Please do not dissolve the reagents at 37 °C directly.
	3. Please carefully reconstitute Standards or working Detection Reagent A and B according to
	the instruction, and avoid foaming and mix gently until the crystals are completely dissolved.
	To minimize imprecision caused by pipetting, use small volumes and ensure that pipettors
	are calibrated. It is recommended to suck more than $10\mu L$ for one pipetting.
	4. The reconstituted Standards, Detection Reagent A and Detection Reagent B can be used only once.
	5. If crystals have formed in the Wash Solution concentrate (30x), warm to room temperature
	and mix gently until the crystals are completely dissolved.
	6. Contaminated water or container for reagent preparation will influence the detection result.

Order at www.antibodies-online.com | www.antikoerper-online.de | www.anticorps-enligne.fr | www.antibodies-online.cn International: +49 (0)241 95 163 153 | USA & Canada: +1 877 302 8632 | support@antibodies-online.com Page 3/5 | Product datasheet for ABIN6953933 | 09/10/2023 | Copyright antibodies-online. All rights reserved.

ot in therange of the standard curve, the optimal sample dilution for the particular iment has to be determined.Samples should then be diluted with PBS (pH =7.0-7.2). say Precision (Precision within an assay): 3 samples with low, middle and high level of vere tested 20 times on one plate, respectively. say Precision (Precision between assays): 3 samples with low, middle and high level of vere tested on 3 different plates, 8 replicates in each plate. SD/meanX100 say: CV < 10% say: CV < 12% earch Use only
iment has to be determined.Samples should then be diluted with PBS (pH =7.0-7.2). say Precision (Precision within an assay): 3 samples with low, middle and high level of vere tested 20 times on one plate, respectively. say Precision (Precision between assays): 3 samples with low, middle and high level of vere tested on 3 different plates, 8 replicates in each plate. SD/meanX100 say: CV < 10%
iment has to be determined.Samples should then be diluted with PBS (pH =7.0-7.2). say Precision (Precision within an assay): 3 samples with low, middle and high level of vere tested 20 times on one plate, respectively. say Precision (Precision between assays): 3 samples with low, middle and high level of vere tested on 3 different plates, 8 replicates in each plate. SD/meanX100
iment has to be determined.Samples should then be diluted with PBS (pH =7.0-7.2). say Precision (Precision within an assay): 3 samples with low, middle and high level of vere tested 20 times on one plate, respectively. say Precision (Precision between assays): 3 samples with low, middle and high level of vere tested on 3 different plates, 8 replicates in each plate.
iment has to be determined.Samples should then be diluted with PBS (pH =7.0-7.2). say Precision (Precision within an assay): 3 samples with low, middle and high level of vere tested 20 times on one plate, respectively. say Precision (Precision between assays): 3 samples with low, middle and high level of
iment has to be determined.Samples should then be diluted with PBS (pH =7.0-7.2). say Precision (Precision within an assay): 3 samples with low, middle and high level of vere tested 20 times on one plate, respectively.
say Precision (Precision within an assay): 3 samples with low, middle and high level of
ot in therange of the standard curve, the optimal sample dilution for the particular
e estimate the concentration of the samples before performing the test. If the values
bilityof causing a deviation due to the introduced chemical substance.The nmended dilution factor is for reference only.
sis buffer is used to prepare tissue homogenates or cell culture supernatant, there is a
minecompatibility with the kit.
sample type is not specified in the instructions, a preliminary test is necessary to
ples should be slowly thawed and centrifuged toremove precipitates.
fore be stored for a short periodat 2 - 8 °C or aliquoted at -20 °C (≤1 month) or -80 °C (≤ nths). Repeated freeze-thawcycles should be avoided. Prior to assay, the frozen
lenaturationmay occur in these samples, leading to false results. Samples should
f r l

Precaution of Use:	The Stop Solution suggested for use with this kit is an acid solution. Wear eye, hand, face, and
	clothing protection when using this material.
Storage:	4 °C/-20 °C
Storage Comment:	 For unopened kit: All reagents should be stored according to the labels on the vials. The Standard, Detection Reagent A, Detection Reagent B, and 96-well Strip Plate should be stored at -20 °C upon receipt, while the other reagents should be stored at 4 °C. For opened kits: the remaining reagents must be stored according to the above storage conditions. In addition, please return the unused wells to the foil pouch containing the desiccant and seal the foil pouch with the zipper.
Expiry Date:	6 months

Order at www.antibodies-online.com | www.antikoerper-online.de | www.anticorps-enligne.fr | www.antibodies-online.cn International: +49 (0)241 95 163 153 | USA & Canada: +1 877 302 8632 | support@antibodies-online.com Page 4/5 | Product datasheet for ABIN6953933 | 09/10/2023 | Copyright antibodies-online. All rights reserved.

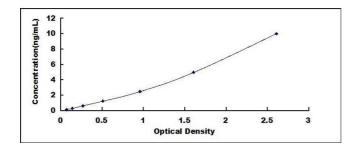

ELISA

Image 1. Typical standard curve

Order at www.antibodies-online.com | www.antikoerper-online.de | www.anticorps-enligne.fr | www.antibodies-online.cn International: +49 (0)241 95 163 153 | USA & Canada: +1 877 302 8632 | support@antibodies-online.com Page 5/5 | Product datasheet for ABIN6953933 | 09/10/2023 | Copyright antibodies-online. All rights reserved.