antibodies - online.com







CFHR1 ELISA Kit





Publication



()	1 /	\sim	KI /	110	Νę
	1//	\vdash	I \/	1 ←	٠// ٢

Quantity:	96 tests	
Target:	CFHR1	
Reactivity:	Human	
Method Type:	Competition ELISA	
Detection Range:	25 ng/mL - 1600 ng/mL	
Minimum Detection Limit:	25 ng/mL	
Application:	ELISA	
Product Details		
Purpose:	For the quantitative determination of human complement factor H-related protein 1 (CFHR1)	
	concentrations in serum, plasma, tissue homogenates.	
Sample Type:	Plasma, Serum, Tissue Homogenate	
Analytical Method:	Quantitative	
Detection Method:	Colorimetric	
Specificity:	This assay has high sensitivity and excellent specificity for detection of human CFHR1. No	
	significant cross-reactivity or interference between human CFHR1 and analogues was	
	observed. Note: Limited by current skills and knowledge, it is impossible for us to complete the	
	cross-reactivity detection between human CFHR1 and all the analogues, therefore, cross	
	reaction may still exist.	
Sensitivity:	12.5 ng/mL	

Product Details

Components:

- Assay plate
- Standard
- HRP-conjugate (100 x concentrate)
- · Sample Diluent
- HRP-conjugate Diluent
- Wash Buffer (25 x concentrate)
- TMB Substrate
- · Stop Solution
- · Adhesive Strip
- · Stop Solution
- Adhesive Strip

Target Details		
Target:	CFHR1	
Alternative Name:	complement factor H-related 1 (CFHR1 Products)	
Background:	Abbreviation: CFHR1 Alias: CFHL, CFHL1P, CFHR1P, FHR1, H36-1, H36-2, HFL1, HFL2, MGC104329, H factor (complement)-like 1 H factor (complement)-like 2 complement factor H-related 1 pseudogene	
UniProt:	Q03591	
Application Details		
Application Notes:	Ontimal working dilution should be determined by the investigator	

Application Notes:		
Sample Volume:		
Assay Time:	1 - 4.5 h	
Plate:	Pre-coated	
Protocol:	1. Prepare reagents, samples and standards as instructed.	
	2. Set a Blank well without any solution.	
	3. Add 50 µL standard or sample to each well.	
	4. Add 50 μL HRP-conjugate (1x) to each well (Not to Blank well).	
	5. Incubate 1 hour at 37 °C	
	6. Aspirate and wash 5 times.	
	7. Add 90 μL of TMB Substrate to each well. Incubate for 20 minutes at 37 °C. Protect from light.	
	8. Add 50 µL Stop Solution to each well. Read at 450 nm within 5 minutes.	

Reagent Preparation:

- 1. HRP-conjugate (1x) Centrifuge the vial before opening. HRP-conjugate requires a 100-fold dilution. A suggested 100-fold dilution is 10 μ L of HRP-conjugate + 990 μ L of HRP-conjugate Diluent.
- 2. Wash Buffer(1x)- If crystals have formed in the concentrate, warm up to room temperature and mix gently until the crystals have completely dissolved. Dilute 20 mL of Wash Buffer Concentrate (25 x) into deionized or distilled water to prepare 500 mL of Wash Buffer (1 x).
- 3. Standard Centrifuge the standard vial at 6000-10000rpm for 30s before opening. Dilute the Standard(10x) with Sample Diluent. A suggested 10-fold dilution is 30 μ L of Standard(10x) + 270 μ L of Sample Diluent. This diluted Standard (S7) serves as the high standard (1600 ng/mL). Do not substitute other diluents. Mix the standard to ensure complete dilution and allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions. Pipette 150 μ L of Sample Diluent into each tube (S0-S6). Use the diluted Standard (S7) solution to produce a 2-fold dilution series (below). Mix each tube thoroughly before the next transfer. Sample Diluent serves as the zero standard (0 ng/mL).

Note:

- Kindly use graduated containers to prepare the reagent. Please don't prepare the reagent directly in the Diluent vials provided in the kit.
- Bring all reagents to room temperature (18-25 °C) before use for 30 min.
- Prepare fresh standard for each assay. Use within 4 hours and discard after use.
- · Making serial dilution in the wells directly is not permitted.
- Distilled water is recommended to be used to make the preparation for reagents.
 Contaminated water or container for reagent preparation will influence the detection result.

Sample Preparation:


- It is recommended to use fresh samples without long storage, otherwise protein degradation and denaturationmay occur in these samples, leading to false results. Samples should therefore be stored for a short periodat 2 8 °C or aliquoted at -20 °C (≤1 month) or -80 °C (≤ 3 months). Repeated freeze-thawcycles should be avoided. Prior to assay, the frozen samples should be slowly thawed and centrifuged toremove precipitates.
- If the sample type is not specified in the instructions, a preliminary test is necessary to determine compatibility with the kit.
- If a lysis buffer is used to prepare tissue homogenates or cell culture supernatant, there is a possibility of causing a deviation due to the introduced chemical substance. The recommended dilution factor is for reference only.
- Please estimate the concentration of the samples before performing the test. If the values are not in therange of the standard curve, the optimal sample dilution for the particular experiment has to be determined. Samples should then be diluted with PBS (pH =7.0-7.2).

Note:

Recommend to dilute the serum or plasma samples with Sample Diluent(1:200) before test. The suggested 200-fold dilution can be achieved by adding 5 μ L sample to 45 μ L of Sample Diluent. Complete the 200-fold dilution by adding15 μ L of this solution to 285 μ L of Sample Diluent. The recommended dilution factor is for reference only. The optimal dilution factor

Application Details

, application because		
	should be determined by users according to their particular experiments.	
Assay Precision:	Intra-assay Precision (Precision within an assay): CV%<8% Three samples of known	
	concentration were tested twenty times on one plate to assess.	
	Inter-assay Precision (Precision between assays): CV%<10% Three samples of known	
	concentration were tested in twenty assays to assess.	
Restrictions:	For Research Use only	
Handling		
Storage:	4 °C,-20 °C	
Storage Comment:	Unopened kit Store at 2 - 8°C. Do not use the kit beyond the expiration date. May be stored for	
	up to 1 month at 2 - 8°C. Coated assay Try to keep it in a sealed aluminum foil plate bag, and	
	avoid the damp. Standard May be stored for up to 1 month at 2 - 8° C. If don't make recent use,	
	better keep it HRP-conjugate store at -20°C. Opened kit HRP-conjugate Diluent Sample Diluent	
	May be stored for up to 1 month at 2 - 8°C. Wash Buffer TMB Substrate Stop Solution *Provided	
	this is within the expiration date of the kit.	
Expiry Date:	6 months	
Publications		
Product cited in:	Staunstrup, Madsen, Primo, Li, Liu, Kragh, Li, Schmidt, Purup, Dagnæs-Hansen, Svensson,	
	Petersen, Callesen, Bolund, Mikkelsen: "Development of transgenic cloned pig models of skin	
	inflammation by DNA transposon-directed ectopic expression of human $\beta 1$ and $\alpha 2$ integrin." in:	
	PLoS ONE , Vol. 7, Issue 5, pp. e36658, (2012) (PubMed).	

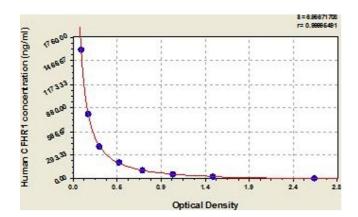

ELISA

Image 1. Typical Standard Curve