

Datasheet for ABIN94333
anti-MICA antibody (Biotin)

3 Images

9 Publications

[Go to Product page](#)

Overview

Quantity:	0.1 mg
Target:	MICA
Reactivity:	Human, Cow, Cat, Non-Human Primate
Host:	Mouse
Clonality:	Monoclonal
Conjugate:	This MICA antibody is conjugated to Biotin
Application:	ELISA, Flow Cytometry (FACS), Immunoprecipitation (IP), Immunocytochemistry (ICC), Immunohistochemistry (Frozen Sections) (IHC (fro))

Product Details

Immunogen:	Membrane of human tonsil cells
Clone:	W6-32
Isotype:	IgG2a
Specificity:	The antibody W6/32 recognises an extracellular epitope of MHC Class I molecules (MHC Class Ia) that are expressed on the surface of all human nucleated cell types. The antibody W6/32 is a valuable reagent for analysing variations in HLA class I expression in different disease states e.g. liver disease, muscular dystrophy, inflammatory myopathy and other neuromuscular disorders. This antibody W6/32 is also suitable as a positive control for HLA tissue typing and crossmatching.
No Cross-Reactivity:	Rabbit
Cross-Reactivity (Details):	Human, Non-Human Primates, Bovine, Feline (Cat)

Product Details

Purification:	Purified antibody is conjugated with biotin LC-NHS ester under optimum conditions and unconjugated antibody and free biotin are removed by size-exclusion chromatography.
---------------	---

Target Details

Target:	MICA
Alternative Name:	HLA-Class I (MICA Products)
Background:	HLA-class I major histocompatibility (MHC) antigens are intrinsic membrane glycoproteins expressed on nucleated cells and noncovalently associated with an invariant beta2 microglobulin. They carry foreign determinants important for immune recognition by cytotoxic T cells, thus important for anti-viral and anti-tumour defence. Human HLA-class I antigens are represented by HLA-A, HLA-B and HLA-C molecules.
Pathways:	Activation of Innate immune Response , Transition Metal Ion Homeostasis

Application Details

Application Notes:	Flow cytometry: Recommended dilution: 1-12 µg/mL
Comment:	The purified antibody is conjugated with Biotin-LC-NHS under optimum conditions. The reagent is free of unconjugated biotin.
Restrictions:	For Research Use only

Handling

Concentration:	1 mg/mL
Buffer:	Phosphate buffered saline (PBS), pH 7.4, 15 mM sodium azide
Preservative:	Sodium azide
Precaution of Use:	This product contains Sodium azide: a POISONOUS AND HAZARDOUS SUBSTANCE which should be handled by trained staff only.
Handling Advice:	Do not freeze. Avoid prolonged exposure to light.
Storage:	4 °C
Storage Comment:	Store at 2-8°C. Do not freeze.

Publications

Product cited in:

Le Discorde, Moreau, Sabatier, Legeais, Carosella: "Expression of HLA-G in human cornea, an immune-privileged tissue." in: **Human immunology**, Vol. 64, Issue 11, pp. 1039-44, (2003) ([PubMed](#)).

Tran, Ivanyi, Hilgert, Brdicka, Pla, Breur, Flieger, Ivasková, Horejsí: "The epitope recognized by pan-HLA class I-reactive monoclonal antibody W6/32 and its relationship to unusual stability of the HLA-B27/beta2-microglobulin complex." in: **Immunogenetics**, Vol. 53, Issue 6, pp. 440-6, (2001) ([PubMed](#)).


Ladasky, Shum, Canavez, Seuáñez, Parham: "Residue 3 of beta2-microglobulin affects binding of class I MHC molecules by the W6/32 antibody." in: **Immunogenetics**, Vol. 49, Issue 4, pp. 312-20, (1999) ([PubMed](#)).

Shields, Ribaldo: "Mapping of the monoclonal antibody W6/32: sensitivity to the amino terminus of beta2-microglobulin." in: **Tissue antigens**, Vol. 51, Issue 5, pp. 567-70, (1998) ([PubMed](#)).

Jacobsen, Aasted, Broe, Petersen: "Reactivities of 20 anti-human monoclonal antibodies with leucocytes from ten different animal species." in: **Veterinary immunology and immunopathology**, Vol. 39, Issue 4, pp. 461-6, (1994) ([PubMed](#)).


There are more publications referencing this product on: [Product page](#)

Images

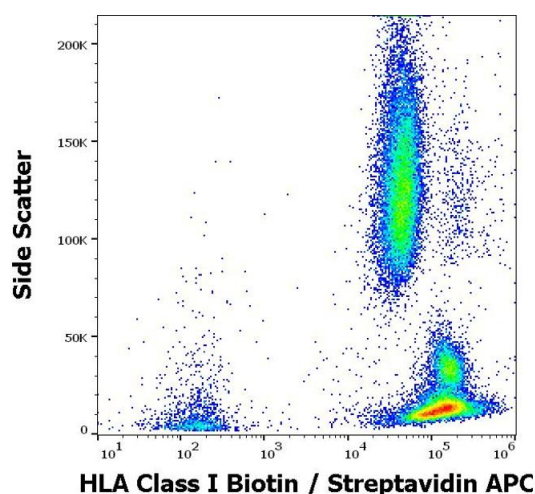

Flow Cytometry

Image 1. Flow cytometry surface staining pattern of human peripheral whole blood stained using anti-human HLA Class I (W6/32) Biotin antibody (concentration in sample 4 µg/mL, Streptavidin APC).

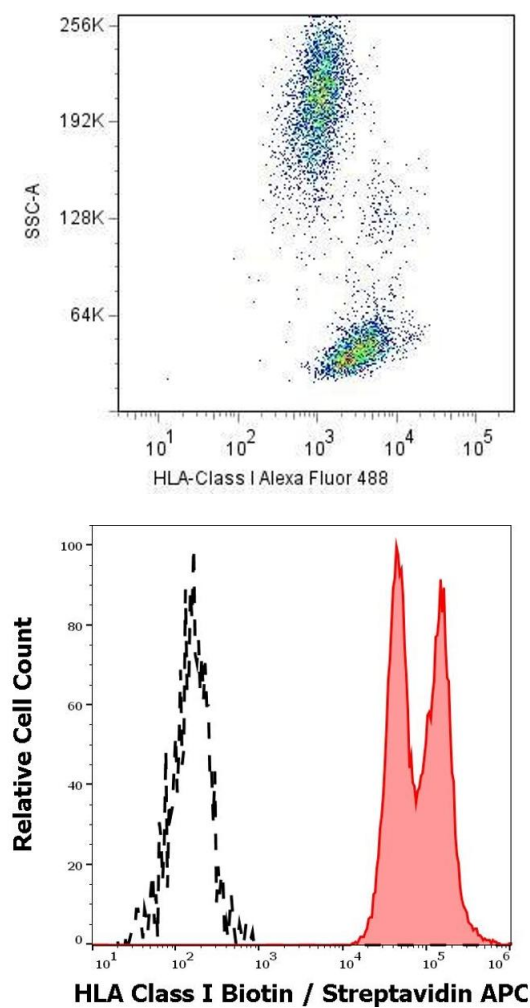

Flow Cytometry

Image 2. Surface staining of human peripheral blood cells with anti-HLA-class I(W6/32) Alexa Fluor® 488.

Flow Cytometry

Image 3. Separation of human leukocytes (red-filled) from HLA Class I negative blood debris (black-dashed) in flow cytometry analysis (surface staining) of human peripheral whole blood using anti-human HLA Class I (W6/32) Biotin antibody (concentration in sample 4 µg/mL, Streptavidin APC).